


# LIDT TEST RESULTS

## LIDT VALUE

|               | Irradiance                              | Linear power density    |
|---------------|---|-------------------------|
| T(120 s)-on-1 | $10.2^{+1.8}_{-1.6}$ MW/cm <sup>2</sup> | $107^{+14}_{-13}$ kW/cm |

NOTE: Each site was exposed to laser radiation for 120 seconds. After each exposure, a waiting period of 240 seconds was applied to allow the sample to cool down.

## DAMAGE PROBABILITY

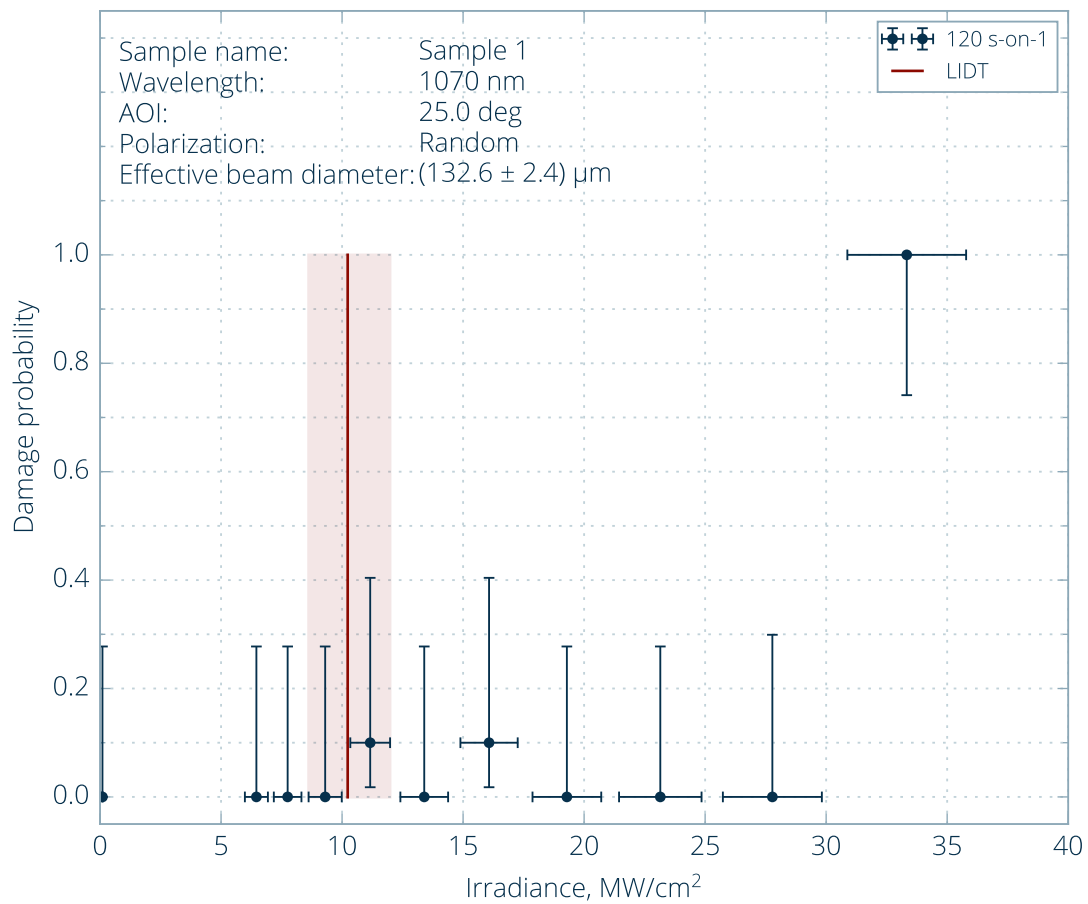

(a) T(120 s)-on-1

Figure 2. Damage probability plot.